

PROGRESS ON THE CRYOGENIC AND CURRENT TESTS OF THE MSU CYCLOTRON GAS-STOPPER SUPERCONDUCTING MAGNET*

M. A. Green, S. S. Chouhan, G. Bollen, J. DeKamp, C. Magsig, and A. F. Zeller, FRIB, and D. Morrissey, J. Ottarson and S. Schwarz, NSCL, MSU, East Lansing, MI 48824, USA

Abstract

The Michigan State University (MSU) cyclotron gas stopper magnet is a warm iron superconducting cyclotron dipole. The desired field shape is obtained by the pole iron profile. Each coil of the two halves is in a separate cryostat and connected in series through a warm electrical connection. The entire system is mounted on a high voltage platform, and is cooled using six two-stage 4.2 K pulse tube coolers. This paper presents the progress on the magnet fabrication, cooling, and current testing.

INTRODUCTION

The fragmentation of fast heavy-ion particles enables fast chemistry-independent production, separation and delivery of exotic isotope beams. The resulting beams have high energies (<100 MeV/A) and large emittances. The range of experiments can be extended by slowing the fast ions, extracting them, and then re-accelerating them. The ReA3 [1] re-accelerator under construction at MSU will reaccelerate thermalized ions (~ 10 keV) to provide low emittance exotic ion beams over a range of energies.

A solution to thermalize and extract light to medium mass beams is to apply a strong gradient dipole magnetic field in a large magnetic gap that forces the ions into a spiral path while slowing them down in He gas at 80 K. Low energy ions near the extraction port are transported in a central extraction orifice by an RF carpet [2], [3]. The ions are transformed into low-energy beams using a differentially pumped ion guide. The low-energy low-emittance beams are transported directly to experiments or to other accelerators for reacceleration. The super-ferric cyclotron gas-stopper magnet at MSU will enable the capture of short-lived rare isotopes.

THE GAS-STOPPER MAGNET

The cyclotron gas-stopper magnet has evolved since it was first proposed in 2007 [4]. The gradient dipole field is produced in a gap of 180 mm between sector cyclotron poles. The peak field in the gap is ~ 2.6 T. A pair of superconducting solenoid coils produce the field. The warm iron poles and flux return can be separated so that the deceleration system can be maintained. Each pole has its own coil and liquid helium cryostat. The two 300 K magnet poles are connected through the iron return path. The coils are not connected at 4 K. Forces to the yoke are transmitted by the cold mass supports. The common axis of the magnet coils is horizontal.

The work reported in this paper was supported in part by an NSF grant PHY-09-58726 and PHY-11-02511.

The space between the poles is evacuated to provide an insulating vacuum for the 80 K magnet beam chamber. Figure 1 shows the assembled magnet with the iron poles closed. Figure 2 shows the magnet poles open. The magnet cryostat on the right has the cylindrical part of the beam chamber vacuum vessel attached. There is a double o-ring seal between the cylindrical portion of the vacuum vessel and the magnet cryostat installed in the left pole piece. One can see the shaped face of the shaped sector cyclotron pole on the pole to the right of Fig. 2.



Figure 1: The assembled magnet is shown fully closed.



Figure 2: The magnet is shown with poles separated. The beam chamber insulating vacuum chamber is visible along with one of the shaped cyclotron poles.

Content from this work may be used under the terms of the CC BY 3.0 licence (© 2015). Any distribution of this work must maintain attribution to the author(s), title of the work, publisher, and DOI.

The nominal design current for the magnet is 200 A. The operating current is expected to be ≤ 180 A. Table 1 shows the cyclotron gas-stopper magnet parameters [5-8]. At both the design current the magnet pole pieces may be somewhat saturated. When the shaped iron poles are not saturated (relative permeability < 100), the magnet self-inductance is nearly constant and lower than when it is with the poles saturated. The self inductance in Table 1 is based on the stored magnetic energy at the magnet design current I_D of 200 A.

Table 1: Cyclotron Gas-stopper Magnet Parameters

Parameter	Value
Iron Pole Radius (m)	1.10
Return Iron Outer Radius (m)	2.00
Average Gap between the Poles (mm)	180
Number of Turns per Coil	1767
Magnet Coil Cross-section R/Z (mm)	80/80
Coil Peak Design Current I_D (A)	200
Peak Design Current Density at I_D ($A\ mm^{-2}$)	54.9
Peak Design Induction in Coil at I_D (T)	2.05
Magnet Peak Stored Energy E_D at I_D (MJ)	3.56
Magnet Self Inductance based on E_D (H)	178
Magnet Cold Mass per Coil (kg)	~ 1240
Magnet Iron Mass (metric tons)	~ 167



Figure 3: The 80 K beam chamber that will be filled with low pressure He gas. (The chamber cover is not shown.)

Figure 3 shows the helium gas filled beam chamber that is cooled to 80 K with liquid nitrogen. The gas slows the ion beam causing it to spiral inward in the gradient dipole field to the center of the chamber.

The magnet cold mass supports are of two types. There are six compression supports that take coil axial forces into the iron. The three radial supports carry gravitational loading and de-centering forces caused by the magnet coil current axis not being the same as the axis of the magnet poles. The cold mass supports are adjustable and their forces are measured during charging.

Even at its design current, the magnet stored-energy is low and the current density in the conductor is low. As a result, the magnet is self quench-protected with long time constant current decays. There is a quench protection system that quenches the magnet in the event of a failure of a lead [9] or when certain system interlocks are triggered. When an event that triggers a rapid discharge is measured, the power supply is disconnected causing the coils to be discharged across a number of 300 K diodes in series. This causes the 4 K diodes [10] across the coils to fire directing the coil current to a resistor wound on the outsides of the coils [6]. When the coil current is 200 A, the coil becomes fully normal within 5 seconds [11].

Each magnet coil is cooled-down and cooled with three Cryomech PT415-RM pulse tube coolers with remote valves and tanks. The helium from the compressors goes through the rotary valves. The rotary valves and the compressors are at ground potential while the coolers and the rest of the magnet may be at ± 50 kV with respect to ground. Figure 4 shows the two magnet cryostats with their coolers. Figure 5 shows the rotary valves and the insulators between the remote valves and the cooler cold heads.



Figure 4: The 4 K cryogenic system for the two cryostats.

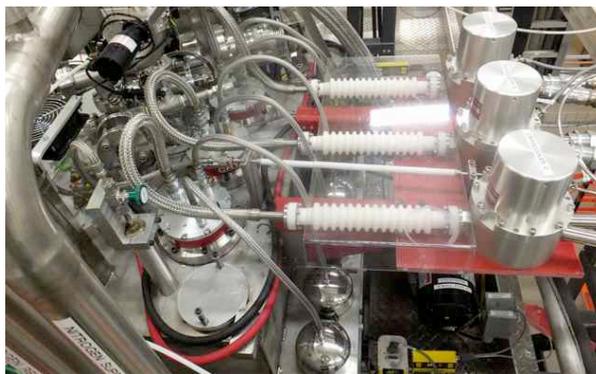


Figure 5: Three cooler cold heads, three 50 kV insulators and three remote valves connected to the compressors.

Each coil has three PT415-RM coolers that each develops ~ 1.35 W of cooling on the second-stage cold head while developing ~ 36 W at 40 K on the first-stage cold head [12]. The first-stage cold heads cool the top of the HTS magnet leads and the 35 K shield around the upper part of the cryostat. The shields around the coils are cooled using liquid nitrogen [13]. Each second-stage cold head has a condenser heat exchanger attached to it.

The three condenser heat exchangers are connected in parallel to a pair of pipes going to the bottom of the magnet coil cryostat and a single pipe coming from the top of the helium reservoir at the top of the cryostat. During 4 K operation there is ~ 12 L of liquid helium in each coil cryostat. The whole circuit is a thermal-siphon cooling loop [14], [15] that can cool-down the 1240 kg magnet cold mass as well as keep it at 4.3 to 4.7 K.

THE MAGNET COOL-DOWN AND POWERING TO 180 A

Magnet Cool-down

The first cool-down of the fixed-side of the magnet started in February of 2014. During the first cool-down a number of problems were uncovered as would be expected the first time a cryogenic system is operated. The insulated pipes bringing helium to the cryostats from the bottles out-gassed clogging the pure helium gas line entering the cryostats. There was some sort of organic crud that froze at ~ 100 K. The insulated pipe was replaced with a pipe that didn't out-gas. Cryostat vacuum problems were also uncovered. The fixed-coil cold mass was cooled to 4 K using three coolers, but it took 3.5 times longer than predicted [16], [17]. The system liquefied helium into the cryostat from warm gas from the high-pressure pure helium gas bottles. Fig. 6 is plot of the temperature in three places on the fixed side coil versus time from the three coolers starting.

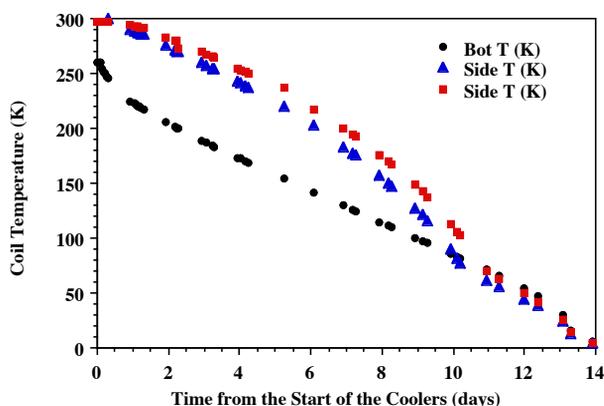


Figure 6: Fixed-coil temperature in three locations as a function of time after the start of the three coolers.

Figure 6 shows that the cool-down time from ~ 297 K to ~ 4 K is about fourteen days once the nitrogen cooled shields are at 80 K. The shields took less than one day to

cool-down. There is some cooling of the helium vessel from the shield through the cold mass supports. The reduced temperature at the bottom of the magnet is due cooling at that point from two of the nine cold mass supports. During the first eight days the three PT415RM coolers provided 75 and 85 W of cooling to the 1240 kg coil cold mass. In terms of the time needed to cool-down the magnet coils, there isn't much difference between the fixed-coils and rolling-coils. The actual cool-down time for both coils was longer than was expected.

The primary reasons for the longer cool-down time for the coils are: 1) the flow passages within the cryostat are smaller than design. 2) There are many more momentum changes within the flow streams. 3) The cryostat helium vessel and flow circuits could not be pressurized above 0.2 MPa. 4) There are unbalanced flows within the flow circuits. 5) The cold mass of each cooling system was larger than 1240 kg. All of these factors will be discussed in a future paper.

Once the magnet was cold and filled, it was clear that the two coil cryostats had very different heat leaks. The fixed-side cryostat has a heat leak of ~ 4.9 W while the rolling-side cryostat has a heat leak of ~ 2.7 W. This will be a topic of a future paper. Both cryostats are at 4.3 to 4.7 K despite having shields at ~ 85 K [13], [18].

Magnet Charging to Full Current

The magnet iron was closed and the two magnet coils were connected in series. The magnet was charged and the forces on the cold mass supports were measured. The cold mass supports were adjusted to balance the magnetic forces on the coils. The magnet quenched a number of times, but there was no quench that originated in either of the coils. All quenches except the last one were caused by interlocks that put warm external diodes across both coils, causing both coils to quench. The final quench at the magnet operating current 180 A was deliberately triggered by putting the warm diodes across the magnet coils. The 180-A quench was like the quench model predicted [11]. It took two days for the two helium vessels to re-fill with liquid helium after the 180-A quench. We have demonstrated that the magnet can operate for long periods of time without quenching.

CONCLUSION

Between late 2013 and mid 2014, the assembly of the MSU cyclotron gas-stopper magnet and its cryogenic system was completed. The magnet coils were cooled down and filled with liquid helium that was liquefied by the coolers from room temperature gas. While the heat load to one cryostat is greater than the heat load to the other, the cooling for both magnet cryostats is acceptable.

The magnet was charged its operating current of 180 A with the iron closed (see Fig. 1). As the magnet was powered, the cold mass supports were adjusted to minimize the unbalanced forces on the magnet cold mass supports. We are nearing off-line beam transport tests (see Fig. 3) now that the magnet is operating routinely.

REFERENCES

- [1] D. Leitner, et al, "Status of ReAccelerator Facility at Michigan State University" *Proceedings MAPAC13, Pasadena CA, USA, FRYBA2*, (2013).
- [2] G. Bollen, et al, *Phys Rev Letters* **96**, 152501 (1996).
- [3] M. Brodeur, et al, "Traveling Wave Ion Transport for the Cyclotron Gas Stopper," *Nucl. Instr. and Meth. in Physic Research B* **317**, pp 468-472 (2013).
- [4] S. S. Chouhan, et al, "Design of a Superferic Cyclotron Gas-stopper Project at NSCL," *2007 Particle Accelerator Conference Proceedings PAC-07*, pp 524-526, (2007).
- [5] S. S. Chouhan, et al, "The Superferic Cyclotron Gas-stopper Magnet Design and Fabrication," *IEEE Trans. on Appl. Supercon.* **23**, No. 3, p 4101805, (2013).
- [6] M. A. Green and S. S. Chouhan, "Cyclotron Gas-stopper Magnet Issues, concerning Lead Stabilization, Magnet Quenching with Diodes and Resistors and a Rapid Discharge System," FRIB Note M40201-CA-000106, 21 May 2013, (not published) This report is available from the first author at green@frib.msu.edu
- [7] S. Schwarz, et al, "The NSCL Cyclotron Gas Stopper – Under Construction," *Nucl. Instr. and Meth. in Physic Research B* **317**, pp 463-467 (2013).
- [8] S. S. Chouhan et al, "Progress on the MSU Superferic Cyclotron Gas-stopper Magnet Quench Protection and Cooling System," *Proceedings of the North American Particle Accelerator Conference NAPAC-13*, Pasadena CA, USA (2013).
- [9] M. A. Green, et al, "Protecting the Leads of a Powered Magnet that is protected with Diodes and Resistors," *IEEE Trans. on Appl. Supercon.* **22**, No. 3, p 4702204, (2012).
- [10] S. S. Chuohan, M. A. Green and A. F. Zeller, "Voltage Characteristics of Diodes used for Passive Quench Protection of Low Current Magnets," "accepted for publication *IEEE Trans. Appl. Supercon.* **25**, No. 3, (2015).
- [11] S. S. Chouhan, M. A. Green and A. F. Zeller, "Simulation of Quenching of the Cyclotron Gas-stopper Magnet at MSU," accepted for publication by *IEEE Trans. Appl. Supercon.* **25**, No. 3, (2015).
- [12] Data sheets for the PT415-RM Cooler produced by Cryomech Inc., 113 Falso Drive, Syracuse NY 13211, USA, <http://www.cryomech.com>
- [13] M. A. Green and S. S. Chuohan, "Cyclotron Gas-stopper Magnet Shield, should it be Cooled with Liquid Nitrogen or should nit be Cooled by the Coolers?" FRIB Note M40201-CA-000108, 21 May 2013, (not published). This report is available from the first author at green@frib.msu.edu
- [14] M. A. Green, et al, "Design Issues for Cryogenic Cooling of Short Period Superconducting Undulators," *Advances in Cryogenic Engineering* **49**, p 783, AIP Press, Melville NY, (2004).
- [15] M. A. Green, "Tests of Four PT-415 Coolers Installed in the Drop-in Mode," co-authored with S. T. Wang, Proceedings ICEC-22 Seoul Korea, 21 to 25 July 2008, p 105, (2008).
- [16] M. A. Green and S. S. Chouhan, "Cyclotron Gas-stopper Magnet Cooling Circuit Pressure Drops and the Cool-down of the Magnet using a Large Refrigerator or Six Two-stage Pulse Tube Coolers," FRIB Note M40201-CA-000107, 21 May 2013, (not published). This report is available from the first author at green@frib.msu.edu
- [17] M. A. Green, S. S. Chouhan, and A. F. Zeller, "Design Limitations on a Thermal Siphon 4 K Helium Loop for Cooling-down the Cyclotron Gas Stopper Magnet Coils," *Advances in Cryogenic Engineering* **59B**, AIP Conference Vol-1573B, pp 1543-1550, AIP Press, Melville NY, (2014).
- [18] M. A. Green, H. Pan, and R. M. Preece, "Changes Made on a 2.7-m Long Superconducting Solenoid Magnet Cryogenic System that allowed the Magnet to be kept cold using 4 K Pulse Tube Coolers," *Advances in Cryogenic Engineering* **59B**, AIP Conference Vol. 1573B, pp 1551-1558, AIP Press, Melville NY, USA (2014).